

UroCure was founded with one goal: to design medical device solutions tailored to address the needs of women and their surgeons.

Our comprehensive portfolio of sling systems—designed to address stress urinary incontinence (SUI) in women—introduces the next generation of devices patterned after the industry standard-bearer, AMS. Each of our products is the result of listening carefully to surgeons, considering the needs of women and designing solutions to deliver the highest quality patient outcomes.

Our sling systems are offered in three configurations to accommodate the surgeon's preferred technique—bottom-up, top-down, or outside-in. Each of our handle-needle designs are noted for their ergonomic design and are optimized for their intended surgical technique. All of our systems incorporate UroCure's best-in-class laser-cut sling with integrated stabilizing suture. This patented innovation helps our sling retain its shape and prevent deformation during placement, tensioning, and sheath removal.

Patient outcomes are critical to our design process: What was her surgical experience? What was her outcome? What can we improve? That is why we are the first sling company to (1) impanel a Quality and Safety Oversight Committee to provide guidance on our commercial path forward, (2) to provide a patient device card with each sling and (3) to offer a means of instantaneous feedback from the OR-to-company via QR code on our product packaging. From start to finish, we are a user-centered company. That is why UroCure sits on the leading edge of women's health.



UroCure slings are distributed exclusively by LiNA Medical USA.

For Customer Service, please call (855) 546-2633 or email info@linamed.com.

Ordering Information:

PART NUMBER:	PRODUCT:	UOM*:
A-TV-1001	UROCURE ArcTV TRANSVAGINAL SLING SYSTEM	INCLUDES ONE (1) ArcTV SLING SYSTEM
A-SP-1001	UROCURE ArcSP SUPRAPUBIC SLING SYSTEM	INCLUDES ONE (1) ArcSP SLING SYSTEM
A-TO-1001	UROCURE ArcTO TRANSOBTURATOR SLING SYSTEM	INCLUDES ONE (1) ArcTO SLING SYSTEM

^{*} Product can only be ordered and shipped in quantities of two

CAUTION: US Federal law restricts this device to sale by or on the order of a physician. This device is intended for use only by physicians with adequate training and experience in the use of polypropylene slings for stress urinary incontinence.

The following adverse events have been reported due to polypropylene mid-urethral sling placement, but are not limited to: Complete failure of the procedure, including worsening of incontinence; partial failure resulting in mild to moderate incontinence; de novo, persistent or worsening overactive bladder and/or detrusor overactivity symptoms, with or without urge incontinence; temporary or permanent lower urinary tract obstruction and retention; tissue responses to the sling implant include; erosion, exposure, extrusion of the mesh through the vaginal or urethral mucosa, bladder wall or other surrounding tissue and/or other organs; scarring / scar contracture / mesh contracture / tissue contraction of vagina or surrounding tissues; device migration; fistula formation and inflammation; dehiscence of vaginal incision; vaginal discharge; an acute or chronic foreign body inflammatory response or infection, which may result in systemic symptoms, pain, damage to adjacent structures, scarring and adhesion; local irritation at the wound site and/or a foreign body response, like all foreign bodies, the polypropylene sling may potentiate an existing infection; allergic reaction to the polypropylene sling; edema and erythema at the wound site; infection (superficial, abscess, systemic sepsis); bleeding (routine surgical, hematoma, hemorrhage); bruising, bleeding, hematoma formation (vaginal, retropubic, abdominal, or thigh); perforation or laceration of vessels, nerves, bladder, urethra or bowel; pain (local or regional) that may be acute or chronic; pain, ongoing pain (pelvic, bladder, vaginal, groin, thigh, suprapubic, dyspareunia, with voiding); severe chronic pain; vaginal shortening or stenosis, which may result in dyspareunia and/or sexual dysfunction; loss of sexual function, temporary or permanent, secondary to pain and/or mesh contracture, tissue contracture or scarring; including inability to have intercourse which may not resolve; pain or discomfort to the patient's partner during intercourse caused by exposed

For further information on indications, contraindications, warnings and precautions, and adverse events refer to the product instructions for use at www.urocure.com/fitu.

UroCure


ADVANCING WOMEN'S HEALTH

701 N 3rd St, Suite 110 | Minneapolis, MN 55401 | www.urocure.com

UroCure


ADVANCING WOMEN'S HEALTH

A PORTFOLIO OF LEADING-EDGE SLING SOLUTIONS

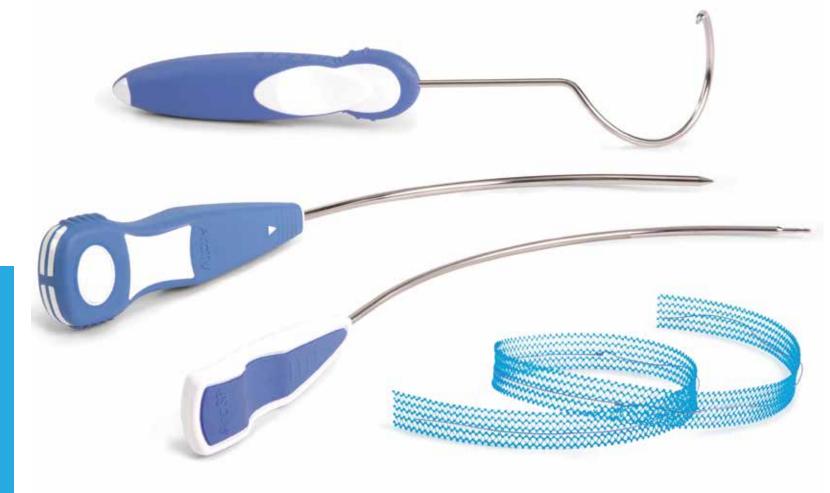


2022 UroCure L.L.C, All rights reserved. UroCure, ArcTV, Equi-Cut and its other trademarks, logos and slogans are the intellectual property of UroCure, L.L.C, and may not be used without permission. | LBL-1001-001 Rev D | SEPT 20

THREE SLING SYSTEMS, ONE GUIDING PRINCIPLE: PATIENT SAFETY AT THE CORE

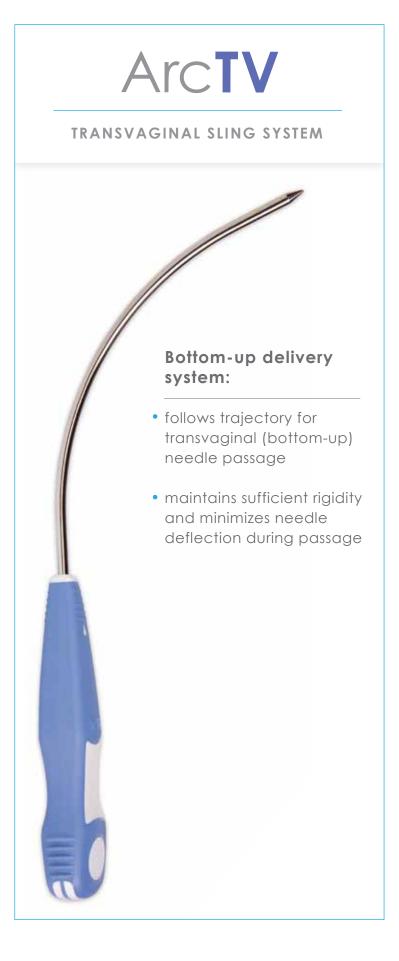




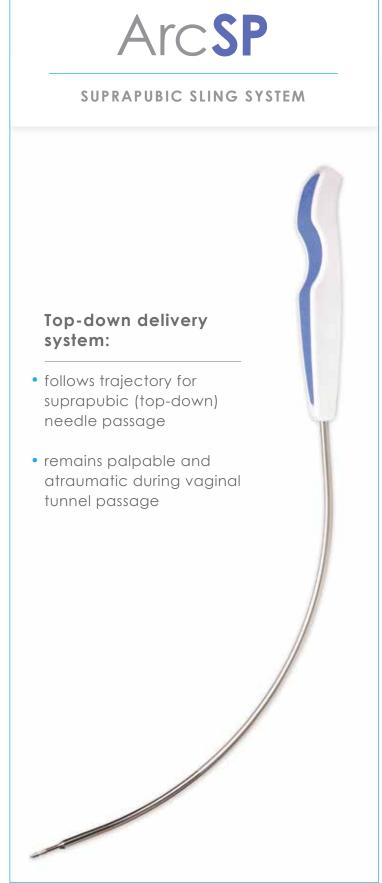


PATENTED SLING WITH STABILIZING SUTURE

Each of our sling systems incorporates UroCure's patented sling with stabilizing suture. Here is why this sling works seamlessly with each of our three needle designs:

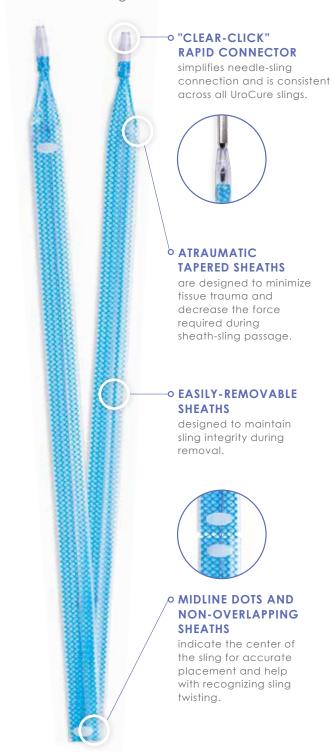



THE STABILIZING SUTURE SETS US APART

Our patented absorbable stabilizing suture was developed in collaboration with leading surgeons and is unique to all UroCure slings. Secured by strategically-placed knots, the suture helps the sling retain its shape—preventing deformation and pore collapse during placement, tensioning, and sheath removal.

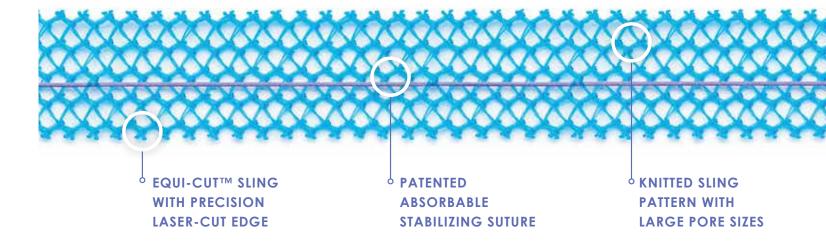


The photos below show how a 7N force, applied to the sling outside the knots, affects the pore integrity of the sling. With the stabilizing suture, the sling experiences minimal stretch and maintains its open pore design. Without the stabilizing suture, the sling experiences severe stretch and pore collapse.

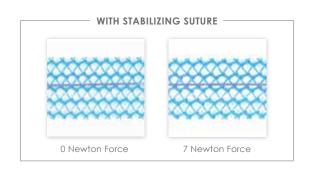

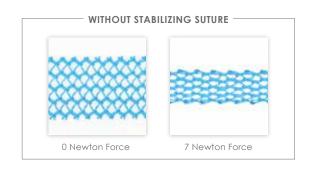

KNOW YOUR IMPLANT—A PATIENT DEVICE CARD

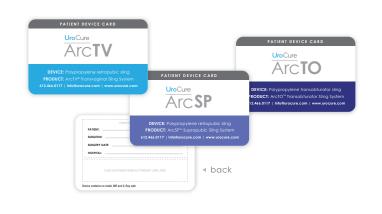

UroCure is the first sling company to include a patient device card with each sling. Patients receive this card during recovery following surgery. Pertinent information included: product name, sling type, device lot number, implant date, surgeon, hospital.